

Agilent N9340B Handheld Spectrum Analyzer (HSA)

3 GHz Technical Overview

Field testing just got easier



Anticipate ____Accelerate ____Achieve




Agilent Technologies

Front panel



Top panel

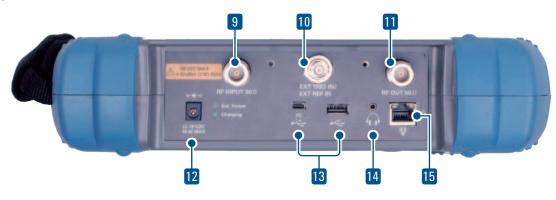

Front panel

- 1. 6.5 TFT display
- 2. Light sensor
- 3. Speaker
- 4. Soft keys
- 5. Back-lit keys
- 6. Power on/off
- 7. Function keys
- 8. Preset

Top panel

- 9. RF INPUT (50 Ω)
- 10. EXT TRIG IN/EXT REF IN
- 11. RF OUT (50 Ω)
- 12. Power input (55 W Max)
- 13. USB connectors
- 14. Headphone connector
- 15. LAN connector

N9340B superior performance ensures the field test confidence

- Superior sensitivity: Lowest DANL in-the-class
- · Fastest sweep time
- Narrowest resolution available
- Frequency range: 100 kHz to 3 GHz (tunable to 9 kHz)¹
- DANL: (RBW = 30 Hz, 10 MHz < fc ≤ 1.5 GHz)
 - ∘ –124 dBm
 - −144 dBm with preamp on
- Sweep time:
 - ° 10 ms to 1000 s, span ≥ 1 kHz
 - < 120 ms at full span
- RBW: 30 Hz to 1 MHz in 1-3-10 sequence
- VBW: 3 Hz to 1 MHz
- SSB Phase noise: < -87 dBc/Hz at 30 kHz offset
- Amplitude accuracy: ± 1.5 dB
- 1. Low frequency performance enhancement options available. Check option N9340B-IBC and N9340B-XDM.

Know your spectrum

Regardless of whether you are handling military communications, a Wireless Service Provider (WSP), or involved with spectrum management you need to avoid impaired communication. The N9340B provides you with a reliable, accurate and detailed picture of your communication spectrum.

Optimize your test time versus accuracy

When you test, you need fast data capture to help locate and identify elusive, transient interference signals. That's why every N9340B spectrum analyzer has a truly fast sweep time. It requires less time to measure across the spectrum, to obtain more reliable test results and to help you achieve more for the same investment of time and money.

Gain confidence in your test results

Spurious signals and noise are of great concern to all network users. A superior combination of low displayed average noise level (DANL) and single sideband (SSB) phase noise coupled with a narrow resolution bandwidth (RBW) means your signal measurements are more reliable and you will have more confidence in your test results. The N9340B's low DANL and SSB phase noise helps you detect very low-level signals (spurs or noise) which are close to the carrier. You will avoid missing these difficult-to-identify signals, which would otherwise lead to an insufficient or even incorrect understanding of the spectrum.

The N9340B's RBW is the narrowest in its class. The narrow 30 Hz bandwidth of the analyzer ensures that it is even easier to identify, resolve, and measure two signals that are close together. Additionally, with a resolution filter shape-factor of less than 5, the N9340B has the ability to resolve closely spaced signals with unequal amplitudes.

Moreover, the narrow RBW means that the spectrum analyzer introduces minimal noise itself, helping to further reduce DANL and improve sensitivity.

Superior sensitivity

With more wireless devices on the market requiring greater bandwidth usage, the ability to discriminate between different signals becomes more challenging. It's under such demanding conditions that the superior performance of an N9340B analyzer proves its worth. The N9340B has one of the best sensitivity and selectivity specifications. The DANL is -124 dBm, or -144 dBm with the optional preamplifier (30 Hz RBW, 10 MHz < fc ≤ 1.5 GHz). The optional preamplifier adds 20 dB gain for improved analyzer sensitivity.

Speed at your fingertips

The RF spectrum is a finite resource, therefore its usage requires management. Most regulatory authorities responsible for administering frequency allocation require service suppliers and network operators to perform routine monitoring of signal power and transmission frequency stability.

N9340B applications for field test

- Aerospace and defence: Radio and radar test, interference analysis, on-site repair
- Wireless service providers: Interference analysis, on-site repair
- TV and broadcasting: Interference analysis, channel power check
- Spectrum management authority: Spectrum monitoring


N9340B is now equipped with powerful features to address field applications using a handheld spectrum analyzer. An analysis is identifying interfering signals. These often arise from illegal transmissions, and may cause impairment of services for authorized users, often resulting in financial loss. These interfering signals could possibly restrict critical communications of civil aviation and emergency services, which could jeopardize public safety.

Spectrogram

Now you can take advantage of the spectrogram display to view the behavior of varying signal parameters over time. The N9340B includes spectrogramas a standard feature. The scrolling three-dimensional display is noted for its ability to track the frequency and power behavior over the time, particularly intermittent signals. The user can use spectrogramto analyze the stability of a signal over the time, or to identify intermittent interference signals in communications systems.

There are two markers for the user to identify power versus frequency and time. Also the time interval between two consecutive colored rows can be adjusted. When amarker is put on the spectrogram, the N9340B can display the trace for the time of the selected marker.

The spectrogramdata and screenshots can be saved and recalled for later analysis or reporting.

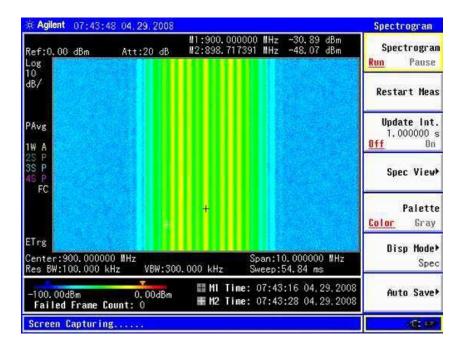

The spectrogram gives the threedimensional display of power, frequency and time.


Extended spectrogrammonitoring (Option INM)

Option INM extends the N9340B spectrogram capability further with the ability to continuously monitor and save spectrogram data over time not only to the analyzer's internal memory or a USB flash drive, but also directly to a PC. With option INM users can save more than 1,500 continuous frames of data depending on the size of the USB flash drive or PC memory.

Option INM also supports an Automatic Save function. The N9340B can save the spectrogram at a user specific time or at a set interval of frame. All the small files with the same prefix can be combined into one file using N9340 PC Software, making analysis easier.

The user can choose among the 3 display modes: spectrogram only, spectrum trace only or the combination of a spectrogram and a spectrum trace in one screen. Limit lines with pass/fail functionality is also available in this measurement. The N9340B will identify the failed frame of spectrogram data with a red mark. The Pass/Fail test can also provide alerts. Users may use marker to find the previous/next frame failed data to quickly find the offending event or interference. The spectrogram data may be played back for review on either the analyzer's display or on a PC utilizing N9340B PC Software.

With the option INM, the Agilent N9340B spectrum analyzer can provide unattended monitoring of communication systems capturing performance or intermittent events like interference over extended periods of time – days rather than hours. The option INMcan provide additional value for the wireless network communication system managers, hospital administrators, etc. as well as police and homeland security by recording spectrogram measurement results over time.

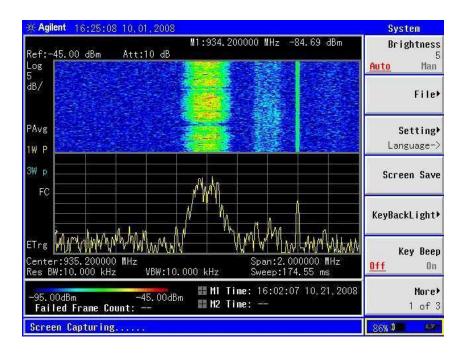

The N9340B INM shows spectrogram and spectrum trace on the same screen.

DSL measurements (Option XDM)


xDSL (ADSL and VDSL) is widely used for broadband internet connections at homes and businesses. Service providers occasionally face problems with interference on their xDSL lines. The interference is mainly intermittent intrusion from nearby external sources such as electric motors, elevators, and appliances. In order to monitor, capture and remove intermittent interference, the engineer may need to work in the field for extended periods of time.

With hardware option XDM the N9340B now supports measurements on ADSL, ADSL2+ and VDSL networks. It provides very good sensitivity with low displayed average noise levels (DANL) to meet the mask requirements over ADSL frequency ranges, from 9 kHz to 12 MHz, for ADSL.

Users may choose t o make the xDSL measurement in either spectrum analysis or spectrogram mode. Using xDSL measurement in spectrogram mode is ideal for capturing intermittent interference on xDSL lines. When used with option INM, the DSL measurement application can measure and record DSL performance data to a USB flash drive or PC over hours or even days.

An xDSL probe from Vierling is required to connect the N9340B analyzer to xDSL networks for measurements in the field.

The option XDM is not available as an upgrade and must be ordered at the time of instrument purchase. The XDM option can also be used for other applications which require improved DANL and phase noise at frequencies from 9 kHz to 12 MHz.

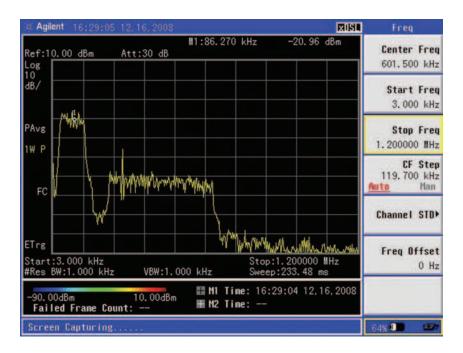

ADSL measurement with N9340B XDM

N9340B IBC also supports a onebutton auto-tune function that greatly simplifies the otherwise complex user setup required to capture and measure IBOC signals of interest. The auto-tune function will automatically set the frequency span, RBW, Average and Detector types, etc. It only takes seconds for the auto-tune function to display the correct measurement results.

The included Channel list feature enables users to easily create and recall setup and measurement parameters for single or multiple broadcast frequencies and channels. The user no longer needs to spend time remembering numerous channel setups but can simply load the desired channel from the list to start a measurement. The Channel list can be loaded, copied and deleted.

N9340B is the industry's first handheld spectrum analyzer with a dedicated IBOC measurement mode. The option IBC is not available as an upgrade and must be ordered at the time of instrument purchase.

IBOC-AM measurement with N9340B IBC


IBOC measurements (Option IBC)

Option IBC equips the N9340B with in-band on-channel (IBOC) measurement capability through a dedicated measurement personality and selected hardware improvements. IBOC technology is a method of transmitting digital and analog radio broadcast signals (AM and FM) simultaneously on the same frequency. This HD Radio[™] version of hybrid digital/analog technology is the only one approved by the FCC for U.S. radio broadcast stations.

The IBC option adds enhanced SSB phase noise for IBOC AM measurements and a noise cancellation process for improved IBOC FM measurement margins. IBOC-AMcovers 530 kHz to 1.7 MHz and IBOC-FMcovers the 87.5 MHz to 108 MHz frequencies.

Option IBC has built-in FCC and NRSC (National Radio Systems Committee) spectral emission masks for quick compliance measurements with visual and audible pass/fail indicators.



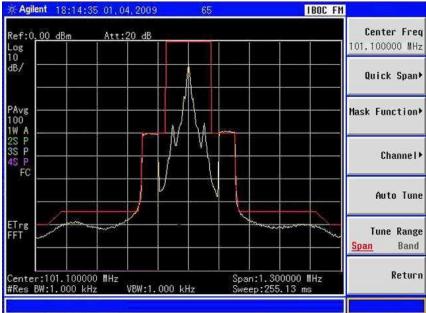

IBOC-FM measurement with N9340B IBC


One-button measurement


The Agilent N9340B supports one-button measurements of occupied bandwidth, channel power and adjacent channel power ratio. This virtually eliminates set-up time in the field.

Occupied bandwidth (OBW)

An occupied bandwidth measurement integrates the power of the displayed spectrum and puts one pair of vertical lines at the frequencies between which the interested signal is contained.

An N9340B spectrum analyzer supports two ways to measure the occupied bandwidth, in percentage or in dBc.

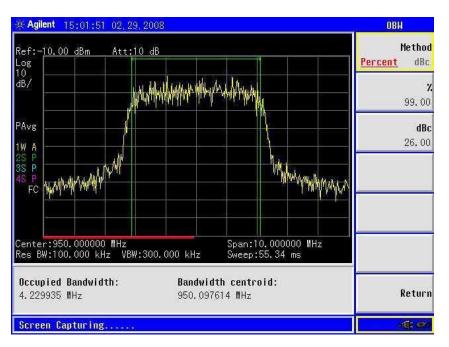

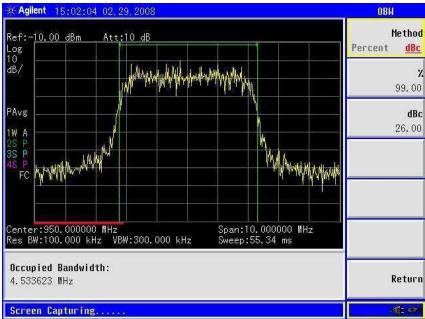


The occupied bandwidth measured in percentage.

The occupied bandwidth measured in dBc.

Channel power


Use channel power to measure both power and power spectral density in a user-specified channel bandwidth. One pair of vertical lines on the display indicates the edges of the channel bandwidth.

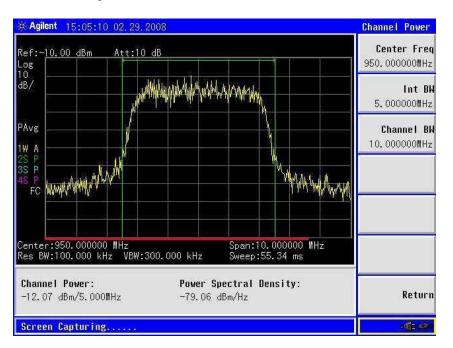

It is quick and easy to set center frequency integration bandwidth, and channel bandwidth.

Adjacent channel power ratio (ACPR)

Wireless service providers need to minimize the interference caused by power leaking into adjacent transmit channels. Adjacent channel power ratio measurements help to check for signal leakage and the identification and control of sources of interference.

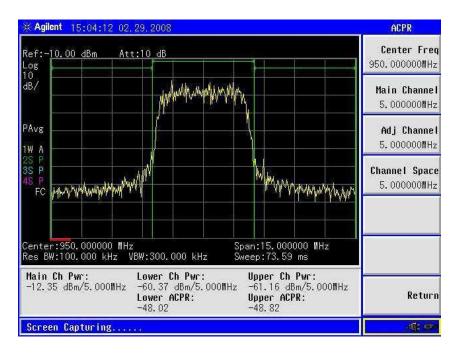


Center frequency, main channel bandwidth, adjacent channel bandwidth, and channel space can eadily be set.

Spectrum emission mask (SEM)

The new N9340B adds Spectrum Emission Mask (SEM) as a standard feature. SEMis a mask for out-of-channel emissions measurement. The SEMis defined relative to in-channel power.

The user can set the parameters of the main channel, out-of-channel frequency bands, and the limit lines. Included is Pass/Fail testing for the overall spectrum emission mask and each individual out-of-channel frequency range. The N9340B will trigger the failure indicator once any measurement result violates the mask.


Also displayed are the main channel power and the power level metrics relative to in-channel power for each out-of-channel frequency range. The user can save the spectrum scan, the mask, the data or screenshot for later analysis and reporting.

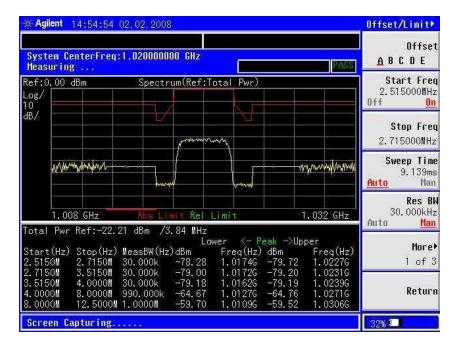


The spectrum emission mask shows the main channel power and the power level vectors relative to in-channel power for each out-of-channel frequency range.

AM/FM modulation analysis (Option AMA)

Optional AM/FM modulation analysis shows the metrics you need, including carrier power, modulation rate, AM depth/FM deviation, SINAD and carrier frequency offset. User definable limits provide Pass/Fail indicators in 4 cases: higher than carrier power, larger than AM modulation index or FM deviation, lower than AM modulation index or FM deviation, or larger than carrier frequency offset. The user can save the waveforms with metrics for reporting as well as the set-up parameters for future measurements or analysis.

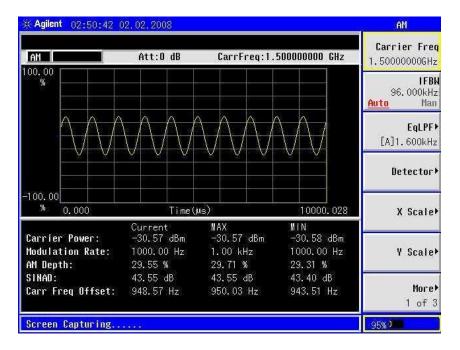

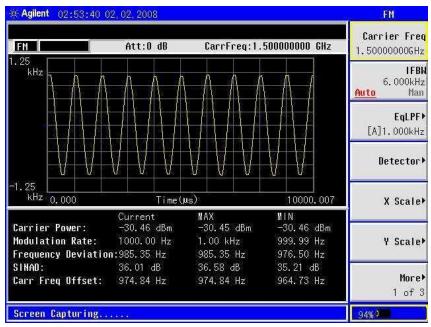


The detailed metrics offer you the complete understanding of the AM.


The detailed metrics offer you the complete understanding of the FM.

ASK/FSK modulation analysis (Option DMA)

Optional ASK/FSK modulation analysis is now available. Amplitude Shift Keying (ASK) is used in RFID and optical systems. Frequency Shift Keying (FSK) is used in many applications including cordless phone, paging system and RFID.

N9340B with option DMA supports 4 display modes: Symbol, Waveform, ASK/FSK Error, and Eye Diagram. Included is Pass/Fail testing of higher than carrier power, higher than ASK modulation depth/FSK frequency deviation, lower than ASK modulation depth/FSK frequency deviation and higher than FSK frequency deviation. The metrics you need are shown, including carrier power, ASK/FSK error, ASK depth/FSK frequency deviation, and ASK index etc. For reports and future measurements the waveform with metrics and setup parameters can be saved.

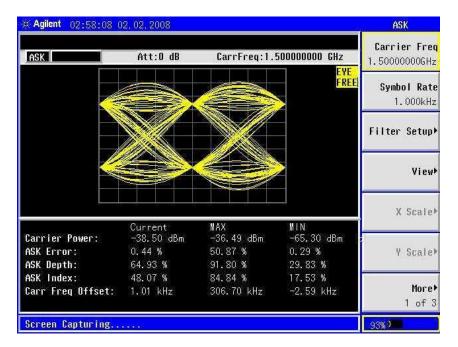

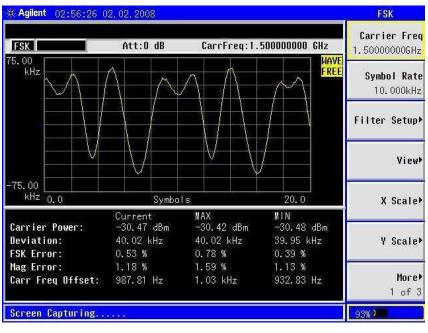

The Eye Diagram of ASK also shows the metrics with detailed parameters.

The Waveform of FSK also shows the metrics with detailed parameters.

High accuracy power measurement

The N9340B now supports high-accuracy, USB plug-and-play power measurements as standard when connected to an Agilent U2000 series USB power sensor. Make true average power measurements for all signal types with wide dynamic range up to 18 GHz with just the push of a button. The Agilent U2000 USB sensors require no external power supplies and with internal zeroing eliminate the need for external calibration. Without the need for additional boxes, the user can easily set up, calibrate and control the power meter/sensor via the analyzer's USB port. The N9340B can collect, display and save the power meter results.

The analyzer also provides Pass/Fail testing with user set upper and lower limits and a Pass/Fail indicator. Test results are shown in dBm and W when making absolute measurements and in dB and percentage when measurements are relative. Two display modes are available: Meter or the Chart mode to log power measurements over time.



N9340B supports Meter and Chart mode to display the results of power measurements.



N9340B supports U2000 series USB power sensors for high accuracy power measurement.

Field strength measurement

Electric field strength measurements are frequently required for field testing of transmitter and antenna coverage. Field strength measurements are now a standard function in the N9340B. Calibrated field strength measurements are easy to make once the antenna factors are loaded into the analyzer via the provided PC software based antenna template. Either field strength (in dB μ V/m, dBmV/m, or V/m) or power flux density (in dBm/m or W/m) can be displayed. With the amplitude offset function, the user can correct gain or loss. And finally together with the user-definable multi-limit line function, the N9340B offers the user quick and convenient field strength measurements and analysis.



The field strength measurement automatically takes into the account of the antenna factor. The antenna table is definable by the standard N9340B PC software.

Channel table

For the users who prefer to tune the spectrum analyzer according to channel numbers rather than center frequency, you will find the new Channel Table feature easy-to-use. The Channel Table includes the major wireless communication standards, such as AMPS, GSM/EDGE/GPRS, CDMA, CDMA2000 etc. The Channel Table can also be edited by the user with the included N9340 PC Software. The revised Channel Table can be downloaded to the analyzer via a PC USB cable or a USB memory stick.

| | 0:52:26 02.0 | | | | Call S | |
|--|--|---|---|---|--|-------------|
| Pat | h: Local | | | | Sil System | D Ty Use |
| Тур | e: STD | | | | · | |
| _ | Name | Tune | Size Modi | fied Time | Loa | ad N |
| CON | 1A2000-NA-Ce | SALES TRANSPORT | 89 2008 | /01/28 11:01 | | _ |
| | ACS_UL ACS_DL | STD STD | | /01/28 11:01 /01/28 11:01 | | Co |
| | 163_0C 1A2000-NA-Ce I | | | /01/28 11:01 | | 10151920 |
| | 1A2000-NA-PC9 1A2000-NA-PC9 | | | /01/28 11:01 /01/28 11:01 | | |
| CDM | 1A2000-TACS_0 | DE STD | 89 2008 | /01/28 11:01 | | Dele |
| | 1A2000-TACS_L 1A-AWS_DL | IL STD Std | | /01/28 11:01 /01/28 11:01 | | |
| CDM | 1a-aws_ul | STD | 59 2008 | /01/28 11:01 | | |
| | 1A-China_DL 1A-China UL | STD STD | | /01/28 11:01 /01/28 11:01 | | |
| | 1A-1 MT2000_DL | 16 (CTALE CTALE) | | /01/28 11:01 | · · | |
| | 1A-1 MT2000_UL 1A-Japan_DL | . STD STD | | /01/28 11:01 /01/28 11:01 | | |
| | 1A-Japan_UL 1A-Japan_UL | STD | 149 2008 | /01/28 11:01 | | _ |
| CDM | 1A-Korea-PCS_ | DL STD | 59 2008 | /01/28 11:01 | | Retu |
| Fre | e: 33380 kByt | e | | | | nc Lu |
| | | 038 | | | | de: |
| | | | | | | |
| lle <u>V</u> iew <u>I</u>) <u>N</u> ew Ì <u>O</u> pen | t the second sec | Trace Data | (*.DAT) (*.JPG) | | | |
|) <u>N</u> ew Open Save Save <u>A</u> s | • Ctrl+S Ctrl+Shift+S | | (*.JPG) (*.MSK) | | | l |
|) <u>N</u> ew Open Save | , Ctrl+S | Trace Data Picture Mask File | (*.JPG) (*.MSK) | | | l |
|) New Open Save Save As Close | Ctrl+S Ctrl+Shift+S Alt+C | Irace Data Picture Mask File Antenna Fil STD File | (*.JPG) (*.MSK) e (*.ANT) (*.STD) | | | |
|) New Qpen Save As Gose Close All Page Setup Page Layou | Ctrl+S Ctrl+Shift+S Alt+C p tt | Irace Data Picture Mask File Antenna Fil STD File | (*,JPG) (*,MSK) e (*,ANT) | | × | |
|) New Qpen Save As Glose Close All Page Setup Page Layou Print Previe | Ctrl+S Ctrl+Shift+S Alt+C p tt | Trace Data Picture Mask File Antenna Fil STD File | (*.JPG) (*.MSK) 9 (*.ANT) (*.STD) dit - AGIELNT-00.ANT | Antenna | Antenna | |
|) New Qpen Save As Close Close All Page Setup Page Layou | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P | Trace Data Picture Mask File Antenna File STD File | (*.JPG) (*.MSK) e (*.ANT) (*.STD) dit - AGIELNT-00.ANT | Factor(dB/m) | Antenna Gain(dBi) | |
| New Open Save Save As Close Close All Page Sgtup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File | (*.JPG) (*.MSK) 9 (*.ANT) (*.STD) dit - AGIELNT-00.ANT | Antenna Factor(dB/m) 23 24.3 | Antenna | |
| New Open Save Save Save Close Close All Page Sgtup Page Layou Print Previe | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File | (*.JPG) (*.MSK) e (*.ANT) (*.STD) dit - AGIELNT-00.ANT Frequncy(MHz) 85 | Factor(dB/m) | Antenna Gain(dBi) -14.21 | |
| New Open Save As Close Close All Page Setup Page Layou Print Previe Brint | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File | (*,JPG) (*,MSK) = (*,ANT) (*,STD) dit - AGIELNT-00.ANT Frequincy(MHz) 85 100 | Factor(dB/m) 23 24.3 | Antenna Gain(dBi) -14.21 -14.1 | 1 |
| New Open Save As Close Close All Page Setup Page Layou Print Previe Brint | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna File STD File | (*,JPG) (*,MSK) (*,MSK) (*,STD) dit - AGIELNT-00.ANT Frequncy(MHz) 85 100 120 150 180 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.58 -14.79 | <u>i</u> |
| New Open Save As Close Al Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture: Mask File Antenna File STD File Antenna E Num 1 2 3 4 5 6 | (*.,PG) (*.MSK) (*.MSK) (*.STD) dit - AGIELNT-00.ANT dit - AGIELNT-00.ANT Frequncy(MHz) 85 100 120 120 150 180. 200 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.58 -14.79 -15.18 | Ĩ |
| New Open Save As Close Close All Page Setup Page Layou Print Previe Brint | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna File STD File Antenna E Num 1 2 3 4 5 6 7 | (*.,PG) (*.MSK) (*.MSK) (*.STD) dit - AGTELNT-00.ANT Frequncy(MHz) 85 100 120 150 180. 200 225 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 | Antenna Gain(dB) -14.21 -14.21 -14.1 -14.12 -14.58 -14.79 -15.18 -15.26 | Į. |
| New Open Save As Close Al Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture: Mask File Antenna File STD File Antenna E Num 1 2 3 4 5 6 | (*.,PG) (*.MSK) (*.MSK) (*.STD) dit - AGIELNT-00.ANT dit - AGIELNT-00.ANT Frequncy(MHz) 85 100 120 120 150 180. 200 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.58 -14.79 -15.18 | Ĩ |
| New Open Save As Close Al Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna File STD File Num 1 2 3 4 5 6 7 8 | (*.,PG) (*.MSK) (*.MSK) (*.STD) dit - AGTELNT-00.ANT frequncy(MHz) 85 100 120 150 130 190 225 250 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 33.5 | Antenna Gain(dB) -14.21 -14.21 -14.12 -14.58 -14.79 -15.18 -15.26 -15.34 | Ĩ |
| New Open Save As Close Close All Page Setup Page Layou Print Previe Brint | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 4 5 6 7 7 8 9 10 11 | (*,PG) (*,MSK) (*,MSK) (*,STD) | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 33.5 30.8 32.4 33.9 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.12 -14.58 -14.79 -15.18 -15.26 -15.34 -11.06 -11.32 -11.66 | Ĩ. |
| New Open Save Save Save Close Close All Page Sgtup Page Layou Print Previe | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 5 6 7 8 9 10 11 11 | (*,3PG) (*,MSK) (*,MSK) (*,STD) dit - AGIELNT-00.ANT Frequincy(MHz) 85 100 120 120 150 100 120 120 120 120 120 120 12 | Factor(dB/m) 23 24.3 25.9 26.3 30.1 31.4 32.5 33.5 30.8 32.4 33.9 36.2 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.12 -14.58 -14.79 -15.18 -15.26 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 | Ĩ |
| New Open Save Save As Close Close All Page Sgtup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 5 6 7 8 9 10 11 11 12 13 | (*,PG) (*,MSK) * (*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) / | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 30.8 32.4 33.9 36.2 38.2 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.12 -14.58 -14.79 -15.18 -15.26 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 -12.44 | 1 |
| New Open Save Save As Close Close All Page Sgtup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 5 6 7 8 9 10 11 11 | (*,3PG) (*,MSK) (*,MSK) (*,STD) dit - AGIELNT-00.ANT Frequincy(MHz) 85 100 120 120 150 100 120 120 120 120 120 120 12 | Factor(dB/m) 23 24.3 25.9 26.3 30.1 31.4 32.5 33.5 30.8 32.4 33.9 36.2 | Antenna Gain(dB) -14.21 -14.1 -14.12 -14.12 -14.58 -14.79 -15.18 -15.26 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 | 1 |
| New Open Save Save As Close Close All Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 4 5 6 7 8 9 9 10 11 11 12 13 14 | (*,PG) (*,MSK) * (*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) /*,STD | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 30.8 32.4 33.9 36.2 38.2 40.1 | Antenna Gain(dB) -14.21 -14.1 -14.1 -14.12 -14.58 -14.79 -15.18 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 -12.44 -13 | 1 |
| New Open Save Save As Close Close All Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 4 5 6 7 8 9 9 10 11 11 12 13 14 | (*,PG) (*,MSK) * (*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) dit - AGIELNT-00.ANT /*,STD) /*,STD | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 30.8 32.4 33.9 36.2 38.2 40.1 | Antenna Gain(dB) -14.21 -14.1 -14.1 -14.12 -14.58 -14.79 -15.18 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 -12.44 -13 | |
| New Open Save Save As Close Close All Page Setup Page Layou Print Previe Print | Ctrl+S Ctrl+Shft+S Alt+C Alt+C o tt Ctrl+Shft+P Ctrl+P | Trace Data Picture Mask File Antenna Fil STD File Antenna Fil STD File Antenna Fil STD File Num 1 2 3 4 4 5 6 7 8 9 9 10 11 11 12 13 14 | (*,PG) (*,MSK) (*,MSK) (*,STD) dit - AGIELNT-00.ANT Frequncy(MHz) 85 100 120 120 120 120 120 200 225 250 300 225 250 300 300 300 300 300 300 300 3 | Factor(dB/m) 23 24.3 25.9 28.3 30.1 31.4 32.5 30.8 32.4 33.9 36.2 38.2 40.1 | Antenna Gain(dB) -14.21 -14.1 -14.1 -14.12 -14.58 -14.79 -15.18 -15.26 -15.34 -11.06 -11.32 -11.66 -12.02 -12.44 -13 | Ĩ |

The channel table offers the ability to tune N9340B according to channel numbers.

The channel table is editable by N9340B PC software.

N9340B optimized usability to enhance field test productivity

- 6.5" TFT screen with bright display for use indoors and outdoors
- · Back-lit keys for night use
- · Four-hour battery life
- Modern USB and LAN connectivity for data transfer and remote control
- Multi-language User Interface
- Rugged design, MIL-PRF 28800F Class 2 compliance



See traces clearly indoors and outdoors

As with all the newest Agilent portable field equipment, operating under challenging bright sunlight or other difficult natural lighting conditions is no problem. The unusual 6.5'' TFT display with resolution of 640 x 480 pixels provides a superior, bright and clear trace for indoor and outdoor use. There is no need to operate in the shade.

Back-lit keys for night use

The N9340B is installed with back-lit keys for night use. The user can see the keys clearly even in darkness. The user can adjust the brightness of keys and the duration of the key light. It offers the user the ability to easily operate N9340B at night.

Built-in light sensor

The N9340B is installed with a light sensor in the front panel. The light-sensor can be activated to adjust the display brightness to adapt to changing lighting conditions.

Long battery life

Testing in the field often means operating away from main power supplies. Batteries need to have the longest possible operating time before recharging. You'll find an Agilent N9340B analyzer has superior power management, providing an impressive 4-hour battery operating time. It's easy to operate for an entire day in the field. There is an advanced, in-built battery management system. This helps extend the useful battery operating time typically up to four hours. With just one battery and a spare, or a quick recharging from any vehicle using the supplied auto-lighter charger, you are able to operate for an entire day away from a mains power source.

Modern USB and LAN connectivity

Remote control N9340B via SCPI over USB/LAN is now available!

Detailed analysis of results in the field is not Remote control N9340B via SCPI over USB/LAN is now available! always convenient or possible. You will need to store the results for later investigation. N9340B supports USB memory stick for data storage and retrival. It makes it easy to transfer and safeguard your measurement data. Connecting to a PC is simple and data transfer is fast via the USB cable. In test lab and bench-top use, the USB/LAN interface and PC software also support PC remote control of Agilent's N9340B spectrum analyzer This allows appropriate use of a large format PC screen. Windows *-compatible software provides automatic storage of selected data and graphics.

Tough enough for the military

You will find that this Agilent analyzer is tough enough for military applications. Apart from its generally compact and rugged construction, the large rubberized grips wrap around both ends, providing additional robust protection from rough handling. The sealed keypad and screen are moisture resistant and dust proof. Of course, there is a protective carrying case that provides further protection for your analyzer.

Multi-language user interface

Users around the world will find operating Agilent N9340B is easy. In addition to English, there are ten more user-selectable, on-screen languages, including Chinese, Japanese, Korean and a number of European languages (see Specifications – General).



N9340B supports remote control via SCPI over USB and LAN.

Specifications

Specifications apply under the following conditions:

- After a warm-up time of 30 minutes, and at least two hours of operation or storage at operating temperature.
- · Within a valid calibration period
- Data with no given tolerances are typical values only. Data designated as 'typical' is not covered by the product warranty.

| Frequency | | Supplemental information |
|--------------------------------|--|--|
| Frequency | | |
| Frequency range | 100 kHz to 3 GHz (tunable to 9 kHz) | AC coupled |
| Internal 10 MHz frequence | y reference accuracy | |
| Aging rate | ± 1 ppm/year | |
| Temperature stability | ± 2 ppm | 0 °C to 30 °C |
| | In addition +2 ppm/10 °C | 30 °C to 50 °C |
| Frequency readout accura | acy with market (Start, stop, center, marker) | |
| Marker resolution | (frequency span)/(number of sweep points -1) | |
| Uncertainty | ± (frequency indication × frequency reference | |
| | uncertainty +1% × span + 20% × resolution bandwidth | |
| | + marker resolution +1 Hz) | |
| | <i>t</i> γ = (aging rate x periond of time since adjustment + tem ₁ | perature stability) |
| Marker frequency counte | | |
| Resolution | 1 Hz | |
| Accuracy | \pm (marker frequency × frequency reference uncertainty | · · · · |
| | + counter resolution) | Noise level > 25 dB; frequency offset 0 Hz |
| | ging rate x periond of time since adjustment + temperatu | re stability) |
| Frequency span | | |
| Range | 0 Hz (zero span), 1 kHz to 3 GHz | |
| Resolution | 1 Hz | |
| Accuracy | ± span/(sweep points – 1) | |
| SSB phase noise | | |
| Carrier offset | | |
| 30 kHz | <87 dBc (1 Hz) | 20 °C to 30 °C; Typical |
| 100 kHz | <-100 dBc (1 Hz) | fc = 1 GHz; RBW 100 Hz; VBW 10 Hz; RMS |
| | | detector |
| 1 MHz | < –120 dBc (1 Hz) | |
| Resolution bandwidth (RE | 3W) | |
| –3 dB bandwidth | 30 Hz to 1 MHz | 1- 3 - 10 sequence |
| Accuracy | ± 5% | Nominal |
| Resolution filter shape factor | < 5 : 1 | 60 dB/3 dB bandwidth ratio; Nominal; |
| | | Digital, approximately Gaussian shape |
| Video bandwidth (VBW) | | |
| –3 dB bandwidth | 30 Hz to 1 MHz | 1-3-10 sequence |
| Accuracy | ± 5% | Nominal |

| Amplitude | | Supplemental information |
|---|---|--|
| Measurement range | | |
| Mododromontrango | Displayed average noise level (DANL) to +20 dBm | |
| Input attenuator range | 0 to 51 dB, in 1 dB steps | |
| Maximum safe input leve | · · | |
| Average continuous power | ≥ +33 dBm; 3 minutes maximum. Nominal | Input attenuator setting \geq 20 dB (input protection switch active when input level > 33 dBm) |
| DC voltage | 50 VDC maximum | · · · · · · |
| Displayed average noise | level | |
| Preamp off | | Reference level ≤ –50 dBm |
| 100 kHz < fc ≤ 1 MHz | < -90 dBm | |
| $1 \text{ MHz} < \text{fc} \le 10 \text{ MHz}$ | < | |
| 10 MHz < fc ≤ 1.5 GHz | < | < -121 dBm when option IBC or XDM is installed |
| $1.5 \text{ GHz} < \text{fc} \le 3 \text{ GHz}$ | < –117 dBm | < –113 dBm when option IBC or XDM is installed |
| fc = 50 MHz | < –126 dBm (Typical) | · |
| fc = 1.9 GHz | < –122 dBm (Typical) | |
| Preamp on | | Reference level ≤ –70 dBm |
| 100 kHz < fc ≤ 1 MHz | < –115 dBm | |
| 1 MHz < fc ≤ 10 MHz | < | |
| 10 MHz < fc ≤ 1.5 GHz | < | < -141 dBm when option IBC or XDM is installed |
| $1.5 \text{ GHz} < \text{fc} \le 3 \text{ GHz}$ | < | < –132 dBm when option IBC or XDM is installed |
| fc = 50 MHz | –146 dBm (Typical) | · |
| fc = 1.9 GHz | -146 dBm (Typical) | |
| RBW = 30 Hz; VBW = 3 Hz; i | nput terminated 50 Ω; 0 dB attenuation; RMS detector; | : Trace average ≥ 40 |
| Level display range | | |
| Log scale and units | 1 to 10 dB/divisions in 1, 2, 5, 10 dB steps, | |
| | 10 divisions displayed | |
| Linear scale and units | 0 to 100%; ten divisions displayed | |
| | dBmV, dBμV, V, mV, μV, W, mW | |
| Sweep (trace) points | 461 | |
| Number of markers | 6 | |
| Marker functions | Normal, frequency counter, noise marker, band power and AM/FM demod (tune and listen) | |
| Marker level readout | Log scale | 0.01 dB |
| resolution | Linear scale | \leq 1% of signal level Nominal |
| Detectors | Normal, Positive Peak, Sample, Negative Peak, Average (Video, RMS, Voltage) | |
| Number of traces | 4 | |
| Trace functions | Clear/write, maximum hold, minimum hold, average | |
| Level measurement error | ± 1.5 dB (excluding input VSWR mismatch) ± 0.5 dB, Typical | 20 to 30 °C, peak detector, preamplifier off, input signal 0 dBm to -50 dBm, 20 dB input attenuation, frequency > 1 MHz, auto sweep time, RBW = 1 kHz, VBW = 1 kHz, trace average on to reduce noise |
| Reference level | | |
| Setting range | –100 to +20 dBm | Steps of 1 dB |
| Setting resolution | | |
| Log scale | 0.1 dB | |
| Linear scale | 1% of reference level | |
| Accuracy | 0 | Because reference level affects only the display not the measurement, it causes no additional error in measurement results from trace data markers |

| Amplitude (continued) | | Supplemental information |
|--|---|--|
| RF Input VSWR (at tuned freque | ency) | |
| Attenuator setting 0 dB | < 1.8 : 1 | 10 MHz to 3.0 GHz, Nominal |
| Attenuator setting 10 dB | < 1.8 : 1 | 100 kHz to 10 MHz, Nominal |
| | < 1.5 : 1 | 10 MHz to 2.5 GHz, Typical |
| | < 1.8 : 1 | 2.5 GHz to 3.0 GHz, Typical |
| Attenuator setting 20 dB | < 1.6 : 1 | 100 kHz to 10 MHz, Nominal |
| | < 1.4 : 1 | 10 MHz to 3.0 GHz, Typical |
| Spurious response | | |
| Second harmonic distortion | <70 dBc | Mixer level = –40 dBm, frequency ≥ 50 MHz |
| Third - order intermodulation (third order intercept) | +10 dBm, Typical | Third-order intermodulation products, 2 x –20 dBm, reference level –10 dBm, center frequency 300 MHz, frequency separation 200 kHz RF attenuation = 0 dB RF preamplifier = 0FF |
| Input related spurious | < -70 dBc | -40 dBm signal at input mixer, carry offset > 1 MHz Exception: -60 dBc nominal (2005.35 MHz) with option XDM or option IBC |
| Inherent residual response | < -88 dBm | Input terminated and 0 dB RF attenuation, preamplifier off, reference level –30 dBm, f > 30 MHz, RBW ≤ 10 kHz |
| Sweep | | Supplemental information |
| Sweep time | | |
| Range | 10 ms to 1000 s | Span ≥ 1 kHz |
| | 6 µs to 200 s | Span = 0 Hz (zero span) |
| Sweep mode | Continuous; single | |
| Trigger source | Free run; video; external | |
| Trigger slope | Selectable positive or negative edge | |
| Trigger delay | | |
| Range | 6 µs to 200 s | |
| Resolution | 6 µs | |
| Front panel input/output RF input | | Supplemental information |
| Connector and impedance | Type -N female; 50 Ω | Nominal |
| 10 MHz reference/External trigg | | |
| Reference input frequency | 10 MHz | |
| Reference input amplitude | 0 to + 10 dBm | |
| Trigger voltage | 5 V TTL level | Nominal |
| Connector and output impendance | BNC female; 50 Ω | Nominal |
| Connectivity | | |
| USB host | USB Type-A female, compatible with USB 2.0 full speed | |
| USB device | USB Type-mini AB female Compatible with USB 2.0 full speed | |
| LAN | RJ-45, 10 Base-T | |
| | | |

| Conorol | | Supplemental information |
|---------------------------|---|--|
| General | | Supplemental information |
| Display | | |
| Resolution | 640 x 480 pixels | |
| Size and type | 6.5 inch (170 mm) TFT color display | |
| Internal memory | | |
| User memory | | Able to store about 3,600 traces |
| Languages | | |
| On-Screen GUI | English, Simplified Chinese, Traditional Chir Russian, Spanish, Portuguese | nese, French, German, Italian, Japanese, Korean, |
| Power requirements and ca | alibration | |
| Adaptor voltage | 90 to 120 or 195 to 263 VAC, 50 to 60 Hz | Auto-ranging |
| | 12 to 18 VDC, < 55 W | |
| Power consumption | 13 W | Typical |
| Battery | | |
| Operating time | 4 hours | Tracking generator off |
| (fully charged battery) | 3 hours | Tracking generator on |
| Charging time | 3 hours | |
| Life time | 300 to 500 charge cycles | |
| Warm-up time | 30 minutes | |
| Environmental and size | | |
| Temperature range | –10 to +50 °C | Operating (Battery: 0 to 50 °C) |
| | -40 to +70 °C | Storage (Battery: -20 to 50 °C) |
| Altitude | 9,144 meters (30,000 feet) | Operating with battery |
| | 3,000 meters (9,840 feet) | Operating with AC to DC adapter |
| | 15,240 meters (50,000 feet) | Non-operating |
| Relative humidity | < 95% | |
| Weight | 3.2 kg (7 lbs) | Net (shipping) approximately |
| - | - · · | 3.5 kg (7.7 lbs) with battery |
| Dimensions | 318 × 207 × 69 mm | Approximately (W x H x D) |
| | | |

| Options | | Supplemental information | |
|---|--|-------------------------------------|--|
| Spectrogram Monitoring (Option I | NM) | | |
| 3 display modes | Spectrogram | | |
| | Spectrum trace | | |
| | Combination of spectrogram and spectrum | trace in one screen | |
| Low frequency performance enhance | ncement and xDSL measurement capa | | |
| XDM channel | 9 kHz to 12 MHz | | |
| DANL | 30 Hz RBW, 3 Hz VBW, 50 Ω termination | | |
| | on input, 0 dB attenuation, RMS detector, | | |
| | Trace Average ≥ 40 | | |
| Preamp off | | Reference level \leq –50 dBm | |
| $9 \text{ kHz} < \text{fc} \le 100 \text{ kHz}$ | < –117 dBm, Nominal | | |
| 10 MHz < fc \leq 12 MHz | < –132 dBm, Nominal | | |
| Preamp on | | Reference level ≤ -70 dBm | |
| $100 \text{ kHz} < \text{fc} \le 1 \text{ MHz}$ | < –138 dBm, Nominal | | |
| $1 \text{ MHz} < \text{fc} \le 12 \text{ MHz}$ | < –140 dBm, Nominal | | |
| Low frequency performance enhance | ncement and AM/FM In-Band On-Cha | annel IBOC Measurement (Option IBC) | |
| Frequency range | | | |
| AM channel | 430 to 1800 kHz | According to IBOC (AM) requirement | |
| FM channel | 87.25 to 108.55 MHz | According to IBOC (FM) requirement | |
| DANL | 30 Hz RBW, 3 Hz VBW, 50 Ω termination | | |
| | on input, 0 dB attenuation, RMS detector, | | |
| | Trace average ≥ 40 | | |
| Preamp off | | Reference level ≤ -50 dBm | |
| $9 \text{ kHz} < \text{fc} \le 100 \text{ kHz}$ | < –117 dBm, Nominal | | |
| $10 \text{ MHz} < \text{fc} \le 12 \text{ MHz}$ | < –132 dBm, Nominal | | |
| Preamp on | | Reference level ≤ –70 dBm | |
| $100 \text{ kHz} < \text{fc} \le 1 \text{ MHz}$ | < –138 dBm, Nominal | | |
| $1 \text{ MHz} < \text{fc} \le 12 \text{ MHz}$ | < –140 dBm, Nominal | | |
| RF preamplifier (Option PA3) | | | |
| Frequency range | 1 MHz to 3 GHz | | |
| Gain | 20 dB | Nominal | |
| Tracking generator (Option TG3) | | | |
| Frequency range | 5 MHz to 3 GHz | | |
| Output level | 0 to –25 dBm | 1 dB steps | |
| Output flatness | ± 3 dB | Referenced to 50 MHz, 0 dBm | |
| VSWR | < 2.0 : 1 | Nominal | |
| Connector and impedance | Type-N female, 50 Ω | | |

| Demodulation | | Supplemental information |
|------------------------------------|---------------------------------|--|
| Frequency range | 10 MHz to 3 GHz | |
| Carrier power accuracy | ± 2 dB | |
| | ± 1 dB | Typical |
| Carrier power displayed resolution | 0.01 dBm | |
| AM measurement | | |
| Modulation rate | 20 Hz to 100 kHz | |
| Accuracy | 1 Hz, nominal | Modulation rate < 1 kHz |
| | < 0.1% modulation rate, nominal | Modulation rate > 1 kHz |
| Depth | 5 to 95% | |
| Accuracy | ± 4% | Nominal |
| FM measurement | | |
| Modulation rate | 20 Hz to 200 kHz | |
| Accuracy | 1 Hz, nominal | Modulation rate < 1 kHz |
| | < 0.1% modulation rate, nominal | Modulation rate > 1 kHz |
| Deviation | 20 Hz to 400 kHz | |
| Accuracy | ± 4% | Nominal |
| ASK measurement | | |
| Symbol rate range | 200 Hz to 100 kHz | |
| Modulation depth/index | | |
| Range | 10% to 95% | |
| Accuracy | ± 4% of reading nominal | |
| Displayed resolution | 0.1% | |
| FSK measurement | | |
| Symbol rate range | 1 kHz to 100 kHz | |
| FSK deviation | | |
| Range | 1 kHz to 400 kHz | |
| Accuracy | ± 4% of reading nominal | $\beta \ge 1$ and $\beta \le 4$ |
| | | ß is the ratio of frequency deviation to symbo |
| | | rate. |
| Displayed resolution | 0.01 Hz | |

Ordering information

| Model number | Description | | |
|---------------------------------|--|--|--|
| N9340B | Handheld spectrum analyzer 100 kHz to 3.0 GHz Accessories supplied as standard with each • Multi-language Quick Start Tutorial | | |
| | | | |
| | | | |
| | CD-ROM of the manual | | |
| | Soft carrying case | | |
| Options | | | |
| N9340B-INM | Extended spectrogram monitoring | | |
| N9340B-XDM | N9340B with low frequency performance enhancement and xDSL measurement capability | | |
| N9340B-IBC | N9340B with low frequency performance enhancement and AM/FM In-Band On-Channel IBOC measurement | | |
| N9340B-PA3 | 3 GHz preamplifier | | |
| N9340B-TG3 | 3 GHz tracking generator | | |
| N9340B-AMA | AM/FM modulation analysis | | |
| N9340B-DMA | ASK/FSK modulation analysis | | |
| N9340B-1TC | Hard transit case | | |
| N9340B-1DN | Automotive 12 V DC charger | | |
| N9340B-BAT | Spare battery pack | | |
| N9340B-ADP | Spare AC/DC adaptor | | |
| N9340B-BCG | External battery charger | | |
| N9340B-TAD | Adaptor Type-N(m) 50 Ω to Type-N (f) 75 Ω DC to 1 GHz | | |
| N9340B-ABA | Manual – English | | |
| N9340B-AB2 | Manual – Chinese | | |
| N9340B-ABJ | Manual – Japanese | | |
| Warranty | | | |
| Select coverage | | | |
| Included | 3-year warranty (return to Agilent), standard | | |
| R-51B-001-5Z | 5-year warranty assurance plan (return to Agilent): | | |
| | Priority warranty service includes one-time coverage for an EOS/ESD failure. | | |
| Calibration | | | |
| Select Agilent calibration plan | | | |
| R-50C-011-3 | 3-year calibration assurance plan (return to Agilent): | | |
| | Priority calibration service covering all calibration costs for 3 years; 15% cheaper than | | |
| | buying stand-alone calibrations. | | |
| R-50C-011-5 | 5-year calibration assurance plan (return to Agilent): | | |
| | Priority calibration service covering all calibration costs for 5 years; 20% cheaper than | | |
| | buying stand-alone calibrations. | | |

www.agilent.com www.agilent.com/find/hsa www.agilent.com/find/n9340b



myAgilent

www.agilent.com/find/myagilent

A personalized view into the information most relevant to you.

Three-Year Warranty



www.agilent.com/find/ThreeYearWarranty

Beyond product specification, changing the ownership experience. Agilent is the only test and measurement company that offers threeyear warranty on all instruments, worldwide.



Agilent Assurance Plans

www.agilent.com/find/AssurancePlans

Five years of protection and no budgetary surprises to ensure your instruments are operating to specifications and you can continually rely on accurate measurements.



www.agilent.com/quality

Agilent Electronic Measurement Group DEKRA Certified ISO 9001:2008 Quality Management System

Agilent Channel Partners

www.agilent.com/find/channelpartners

Get the best of both worlds: Agilent's measurement expertise and product breadth, combined with channel partner convenience.

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at: www.agilent.com/find/contactus

Americas

| Canada Brazil Mexico | (877) 894 4414 (11) 4197 3600 01800 5064 800 |
|----------------------------|--|
| United States | (800) 829 4444 |
| Asia Pacific | |
| Australia | 1 800 629 485 |
| China | 800 810 0189 |
| Hong Kong | 800 938 693 |
| India | 1 800 112 929 |
| Japan | 0120 (421) 345 |
| Korea | 080 769 0800 |
| Malaysia | 1 800 888 848 |
| Singapore | 1 800 375 8100 |
| Taiwan | 0800 047 866 |
| Other AP Countries | (65) 375 8100 |
| | |

Europe & Middle East

| Belgium | 32 (0) 2 404 93 40 |
|----------------|----------------------|
| Denmark | 45 45 80 12 15 |
| Finland | 358 (0) 10 855 2100 |
| France | 0825 010 700* |
| | *0.125 €/minute |
| Germany | 49 (0) 7031 464 6333 |
| Ireland | 1890 924 204 |
| Israel | 972-3-9288-504/544 |
| Italy | 39 02 92 60 8484 |
| Netherlands | 31 (0) 20 547 2111 |
| Spain | 34 (91) 631 3300 |
| Sweden | 0200-88 22 55 |
| United Kingdom | 44 (0) 118 927 6201 |
| | |

For other unlisted countries:

www.agilent.com/find/contactus (BP-09-27-13)

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 2014 Published in USA, February 11, 2014 5989-7847EN



Agilent Technologies