

HIOKI

60000

99999

HIOKI

60000

99999

HIOKI

5000

5000.



99 Washington Street Melrose, MA 02176 Phone 781-665-1400 Toll Free 1-800-517-8431



DMM

Visit us at www.TestEquipmentDepot.com

DIGITAL MULTIMETER DT4200 Series

Super Fast Response Rate and Safety Features Take Professional Testing to a Higher Level

High-End Models Standard Models Pocket Models

DT4281 / 4282 DT4251 / 4252 / 4253 DT4221 / 4222

HIOKI

6000

5000.

HIOKI

6000

5000 -

нокі

6000



HOK

6000



ISO 9001 ISO14001 HIOKI company overview, new products, environmental consideration and other information are available on our website

www.valuetronics.com



DMMs For **Every Application**

To Be The World's Fastest

DT4280/4250/4220 Series Features




The world's fastest DMM engine

In striving to offer the world's fastest measurement response in a DMM, the custom ASIC is developed in-house at Hioki, allowing us to embody the concentration of our technological strengths.



Nearly 0.6 s measurement response

Get a stable reading in about half a second from probe contact to display. See for yourself how fast it really is with the DT4250 and DT4220 Series.



current valu

Absolutely Reliable True RMS





The True RMS method provides the best accuracy.



Operator Safety

Safety is our priority. Terminal shutters in the DT4280 Series and other safety features assist in preventing accidents to the operator and damage to the instrument.



Shock and Dust Resistant

Protective rubber edges around the DMM endure drop from 1 meter onto a concrete floor and a precise design shields against dusty environments.





Bright Backlight

The super bright LED backlight is indispensable in dark locations to clearly capture the measured values. (Red LED backlight available only in the DT4280 series

High-End

High accuracy, additional function enhancements, broad range of measurement items



www.valuetronics.com

For those with diverse measurement needs

DT4200 Series Basic Comparison

		-			1		
	DT4281	DT4282	DT4251	DT4252	DT4253	DT4221	DT4222
Basic Characteristics							
True RMS	Ye	s	Yes			Yes	
DCV basic accuracy	±0.025 %rc	lg. ±2 dgt.		±0.3 %rdg. ±5 dgt.		±0.5 %r	dg. ±5 dgt.
Measurement items (Ty	pical ranges are indica	ated; may not reflect i	maximum or minimu	m measurable signal)			
DC voltage	60mV to	1000V		600mV to 1000V		600m\	' to 600V
AC voltage	60mV to	1000V		6V to 1000V		6V te	o 600V
DCV + ACV	6V to 1	000V		n/a		r	n/a
DCA current	600µA to 600mA	600µA to 10A	n/a	6A to 10A	60µA to 60mA	r	n/a
ACA current	600µA to 600mA	600µA to 10A	n/a	6A to 10A	n/a	r	n/a
AC clamp	10A to 1000A	n/a	10A to 1000A	n/a	10A to 1000A	r	n/a
Resistance	60Ω to 6	600MΩ		600Ω to $60M\Omega$		n/a	600Ω to $60M\Omega$
Temperature	-40°C to	800°C	n/a	n/a	-40°C to 400°C	r	n/a
Capacitance	1nF to 1	I00mF		1µF to 10mF		n/a	1µF to 10mF
Frequency	99Hz to	500kHz		99Hz to 99kHz		99Hz t	o 9.9kHz
Continuity check	Ye	s		Yes		١	′es
Diode check	Ye	s		Yes		n/a	Yes
Conductance	n/a	Yes		n/a		r	n/a
Voltage detection	n/	a	Yes	n/a	n/a	Yes	n/a
Additional Functions							
AUTO AC/DCV	n/	a	Yes	n/a	Yes	Yes	n/a
Peak measurement	DC/	AC		n/a		r	n/a
Low-pass filter	Analog filter		Digital filter			Digit	al filter
•	Cut-off :		Pass-band : 100Hz/500Hz				: 100Hz/500Hz
Display update setting	Ye	-	n/a				n/a
Hold display value	AUTO / N		AUTO / MANUAL				NUAL
Max/Min value display	Ye	-		Yes			n/a
Relative display	Ye	S	Yes				és
Decibel conversion	Ye	s		n/a	1	r	n/a
Percentage conversion display	Ye	S	n/a	n/a	Yes	r	n/a
Data storage							
Capacity	Max 40	0 data		n/a		r	n/a
USB communication*1	Ye	S	Yes			r	n/a
Operating time							
Continuous operating time	Approx. 10		Approx. 130 hours			Approx	40 hours
Power supply	Alkaline (LR6) battery ×4 / M	anganese(R6P) battery ×4	Alkaline (LR03) battery ×4			Alkaline (LR	03) battery ×1
Display							
Back light	Ye	S	Yes				⁄es
Dual display	Ye	s		Yes		r	n/a
Bar graph display	n/	a		Yes		١	′es
Safety							
Safety standard categories	CAT Ⅲ1000V	/ CAT IV 600V	C	AT III 1000V/ CAT IV 60	VOC	CAT 111 600	// CAT IV 300V
Mis-insertion prevention shutters	Ye	S	n/a			r	n/a

*1. Requires optional DT4900-01 Communication Package

*2. When using four AA alkaline batteries

Glossary


Auto AC/DCV	Automatically detects and measures AC and DC voltage.		
Peak measurement	After starting PEAK value measurement, check maximum and minimum instantaneous voltage and current values.		
Low-pass filter	Cuts high frequency content to provide stable numerical values for measurement.		
Display update setting	Reduces the display value update rate to stabilize measurements.		
Hold display value	Manual: press the button to freeze the display. Auto: the display freezes automatically when the measurement value is stable.		
Max/Min value display	Pressing the MAX/MIN button displays the maximum and minimum displayed measurement values.		
Relative display	Pressing the REL button displays subsequent measurements as values relative to that displayed when the button was pressed.		
Decibel conversion	Displays AC voltage measurements converted to decibel values (dbm/dbv)		
Percentage conversion display	Displays 4 to 20 mA (or 0 to 20 mA) signals converted to 0 to 100% values. For the DT4253, only 4 to 20 mA.		

Why are there no current measurement terminals on some of the models?

Hioki's new digital multimeter series include models with no directly accessible current measuring terminals. These models reflect our mission to provide the highest level of safety in a DMM.



Size Comparison

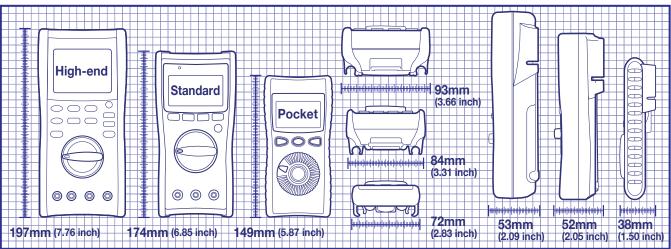

DT4281/DT4282

Display




Typical waveform +harmonic components

Ideal for checking ripple voltage in DC supply systems

Peak measurement function & DC+AC voltage measurement

Typical waveform component

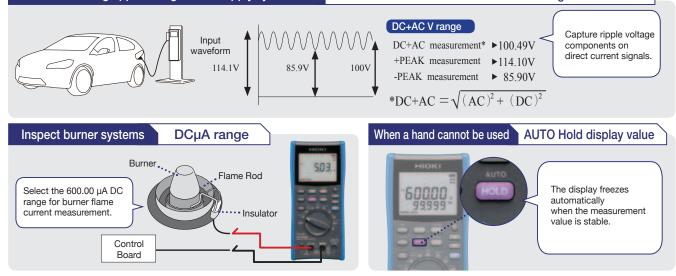

Accuracy Guaranteed for 1 Year @ $23\pm5^{o}C~(73^{o}F\pm41^{o}F)$, 80% RH or less (no condensation)

DC Voltag	je		
Range	Accuracy	Input Impedance	
60.000 mV	±0.2 %rdg. ±25 dgt.	100	
600.00 mV	±0.025 %rdg. ±5 dgt.	$1G\Omega$ or more	
6.0000 V	±0.025 %rdg. ±2 dgt.	11.0ΜΩ	
60.000 V	±0.023 %idg. ±2 dgl.	10.3ΜΩ	
600.00 V	±0.03 %rdg. ±2 dgt.	10.2ΜΩ	
1000.0 V	±0.03 %idg. ±2 dgt.	10.210122	

AC Voltage						
Range			Ac	curacy		
Kange	20 to 45Hz	45 to 65Hz	65 to 1kHz	1k to 10kHz	10k to 20kHz	20k to 100kHz
60.000 mV	±1.3 %rdg.	±0.4 %rdg.	±0.6 %rdg.	±0.9 %rdg.	±1.5 %rdg.	±20 %rdg. ±80 dgt.
600.00 mV	±60 dgt.	±40 dgt.	±40 dgt.	±40 dgt.	±40 dgt.	±8 %rdg. ±80 dgt.
6.0000 V	±1 %rdg. ±60 dgt.				±0.7 %rdg. ±40 dgt.	±3.5 %rdg. ±40 dgt.
60.000 V		±0.2 %rdg. ±25 dgt.	±0.3 %rdg.	±0.4 %rdg. ±25 dgt.	±40 ugi.	±40 ugi.
600.00 V 1000.0 V	Undefined		±25 dgt.		Undefined	Undefined

DCV + ACV Measurement

Range			Ac	curacy				
Range	20 to 45Hz	45 to 65Hz	65 to 1kHz	1k to 10kHz	10k to 20kHz	20k to 100kHz		
6.0000 V	±1.2 %rdg. ±65 dgt.			±0.4 %rdg.	±1.5 %rdg. ±45 dgt.	±3.5 %rdg. ±125 dgt.		
60.000 V		±0.3 %rdg.	±0.4 %rdg.	±30 dgt.	±45 dgt.	±125 ugt.		
600.00 V	Undefined	±30 dgt.	±30 dgt.					
1000.0 V			±0.4 %rdg. ±45 dgt.	Undefined	Undefined			
Input impe	dance	$1M\Omega \pm 4\%$	$1M\Omega \pm 4$ %//100pF or less					
Crest factor 3 or less (1.5 or less for the 1000.0V			he 1000.0V ra	ange)				
Accuracy		5% or more of each range						
specificatio	n range	With the filter ON, accuracy is defined only for frequencies 100Hz or less. Furthermore, 2% rdg. is added						

DCA Measu	rement	6A, 10A rar	ige : DT4282 only	
Range	Accuracy / Display update : SLOW	Accuracy / Display update : NORMAL	Shunt Resistance	
600.00 μA		±0.05 %rdg. ±25 dgt.	101 Ω	
6000.0 μA	±0.05 %rdg. ±5 dgt.	±0.05 %rdg. ±5 dgt.	101 22	
60.000 mA		±0.15 %rdg. ±25 dgt.	1.0	
600.00 mA	±0.15 %rdg. ±5 dgt.	±0.15 %rdg. ±5 dgt.	1 22	
6.0000 A	±0.2 %rdg. ±5 dgt.	±0.2 %rdg. ±25 dgt.	10m Ω	
10.000 A	±0.2 %10g. ±5 dgt.	±0.2 %rdg. ±5 dgt.	10111 12	

$\begin{array}{c} & & & & \\ 600.00 \ \mu A & & \pm 1 \\ \hline 6000.0 \ \mu A & & \pm 1 \end{array}$	ment 0 to 45Hz .0 %rdg. .20 dgt. .0 %rdg. ±5 dgt.	45 to 65Hz ±0.6 %rdg. ±20 dgt. ±0.6 %rdg.	6A Accuracy 65 to 1kHz ±0.6 %rdg. ±20 dgt.	10A range : 1k to 10kHz ±2 %rdg.	DT4282 only 10k to 20kHz ±4 %rdg.
$\begin{array}{c c} & & 20 \\ \hline & & & \\ \hline 600.00 \ \mu A \\ \hline & \pm 1 \\ \hline & & \\ \hline 6000 \ 0 \ \mu A \\ \hline \end{array}$.0 %rdg. =20 dgt. .0 %rdg.	±0.6 %rdg. ±20 dgt.	65 to 1kHz ±0.6 %rdg.		
$\begin{array}{c c} & & 20 \\ \hline & & \\ 600.00 \ \mu A \\ \hline & \pm 1 \\ \hline & \\ 6000 \ 0 \ \mu A \\ \end{array} $.0 %rdg. =20 dgt. .0 %rdg.	±0.6 %rdg. ±20 dgt.	±0.6 %rdg.		
600.00 μA ±1	±20 dgt.	±20 dgt.	0	±2 %rdg.	+4 %rda
6000 0 µA ±1	.0 %rdg.		±20 dgt.		0
6000 0 HA I		±0.6 %rda		±20 dgt.	±20 dgt.
0000.0 μΛ	±5 dgt.	±0.0 %10g.	±0.6 %rdg.	±2 %rdg.	±4 %rdg.
		±5 dgt.	±5 dgt.	±5 dgt.	±5 dgt.
60.000 mA ±1	.0 %rdg.	±0.6 %rdg.	±0.6 %rdg.	±1 %rdg.	±2 %rdg.
±	±20 dgt.	±20 dgt.	±20 dgt.	±20 dgt.	±20 dgt.
600 00 mA ±1	.0 %rdg.	±0.6 %rdg.	±0.6 %rdg.	±1.5 %rdg.	Undefined
000.00 IIIA	±5 dgt.	±5 dgt.	±5 dgt.	±10 dgt.	Undernied
6.0000 A U	Indefined	±0.8 %rdg.	±0.8 %rdg.	Undefined	Undefined
0.0000 A 0	Indenned	±20 dgt.	±20 dgt.	Undenned	Ondenned
10.000 A U	Indefined	±0.8 %rdg.	±0.8 %rdg.	Undefined	Undefined
10.000 A 0	Indenned	±5 dgt.	±5 dgt.	Ondennied	Ondennied
Shunt resistance	ŀ	uA Range 101Ω/	mA Range 1Ω/ A	Range $10m\Omega$	
Crest factor	Crest factor 3 or less (Note that it applies to 1/2 of the range.)				
Accuracy specification range Accuracy is not defined for measurements below 5% of range					of range
Continuity Check					

Range	;	Accuracy		Measurement Curren	t Open-terminal Voltage		
600.0 9	±0.5 %rdg. ±5 d	gt.	$640~\mu A{\pm}10\%$	2.5 V DC or less			
Continuity threshold 20Ω (default) /50 Ω / 10			2/100	Ω/ 500Ω			
Diode Check							
Range	1	Accuracy	Mea	asurement Current	Open-terminal Voltage		
3.600 V	±0.1 %rdg. ±5 dgt.		1	.2 mA or less	DC4.5 V or less		
Forward threshold If the		5V/ 0.5V (default)/1V/ 1.5V/ 2V/ 2.5V/ 3V					
		the reading is lower than the threshold during the forward connection, buzzer sounds and the red backlight turns on.					
Peak Measure	ement (For	AC V, DC V, DC+AC V,	Clam	p, DC μA, DC mA, D	C A, AC μA, AC mA, AC A)		
Main measurement		Signal width			Accuracy		
DCV 4r		4ms or more (single)		±2.0	%rdg. ±40 dgt.		
DCV	1ms or more (repeated)			±2.0 %	±2.0 %rdg. ±100 dgt.		
Other than	1m	is or more (single)	_	±2.0	±2.0 %rdg. ±40 dgt.		
DCV	250µs or more (repeated)			±2.0 %	±2.0 %rdg. ±100 dgt.		

Decibel Conversion Measurement : Standard impedance (dBm) 4/8/16/32/50/75/93/110/125/135/150/200/250/300/500/600/800/900/1000/1200 Ω (default : 600 Ω)

AC Clamp (AC	Current)			D14281 On	
Danas		Acc	curacy		
Range	40 to 65Hz		65	to 1kHz	
10.00 A	±0.6 %rdg. ±2 dgt.		±0.9 %rdg. ±2 dgt.		
20.00 A	±0.6 %rdg. ±4 dgt.		±0.9 %rdg. ±4 dgt.		
50.00 A	±0.6 %rdg. ±10 dgt.		±0.9 %	rdg. ±10 dgt.	
100.0 A	±0.6 %rdg. ±2 dgt.		±0.9 %	ordg. ±2 dgt.	
200.0 A	±0.6 %rdg. ±4 dgt.		±0.9 %	ordg. ±4 dgt.	
500.0 A	±0.6 %rdg. ±10 dgt.		±0.9 %	rdg. ±10 dgt.	
1000 A	±0.6 %rdg. ±2 dgt.		±0.9 %	ordg. ±2 dgt.	
Crest factor Accuracy is not de	t include the error of the clan 3 or less efined for measurements belo	1 1			
Resistance Me Range	Accuracy		Measurement Current	Open-terminal Voltag	
60.000 Ω	±0.3 %rdg. ±20 dgt.	,		1 0	
600.00 Ω	±0.03 %rdg. ±10 dgt.		$640~\mu A{\pm}10\%$		
6.0000 kΩ	0 0		96 µA±10%	1	
60.000 kΩ	±0.03 %rdg. ±2 dgt.		9.3 μA ±10%	1	
600.00 kΩ			0.96 µA±10%	DC2.5 V or les	
6.0000 MΩ	±0.15 %rdg. ±4 dgt.			1	
60.00 MΩ	±1.5 %rdg. ±10 dgt.	0 0			
(00.0.)(0	±3.0 %rdg. ±20 dgt.		96 nA ±10%		
600.0 MΩ	±8.0 %rdg. ±20 dgt.				
Conductance (nS)			DT4282 on	
Range	Accuracy	Meas	surement Current	Open-circuit Voltag	

AC Clamp (AC Curr

Capacitance	Measurement			
Range	Accuracy	Measurement Current	Open-circuit Voltage	
1.000 nF	±1.0 %rdg. ±20 dgt.			
10.00 nF		32 μA ±10%	DC2 5 V or less	
100.0 nF	±1.0 %rdg. ±5 dgt.	52 µA ±1070	DC2.5 V OI less	
1.000 µF				
10.00 µF			DC3.1 V or less	
100.0 µF	±2.0 %rdg. ±5 dgt.		DC3.1 V OI less	
1.000 mF		680 μA ±20%		
10.00 mF			DC2.1 V or less	
100.0 mF	±2.0 %rdg. ±20 dgt.			

Temperature Thermocouple Type Range K -40.0 to 800.0 °C (-40.0 to 1472.0°F) ±0.5 %

 K
 -40.0 to 800.0 °C (-40.0 to 1472.0°F)
 ±0.5 %rdg. ±3 °C (5.4°F)

 The optional K Thermocouple DT4910 is used. Accuracy does not include the error of the K thermocouple
 The optional K Thermocouple DT4910 is used. Accuracy does not include the error of the K thermocouple

Accuracy

Frequency (Fo	Frequency (For AC V, DC+AC V, AC μA, AC mA, AC A)				
Range	Accuracy				
99.999 Hz					
999.99 Hz	±0.005 %rdg. +3 dgt.				
9.9999 kHz					
99.999 kHz	10.005.07 1. 12.17				
500.00 kHz	±0.005 %rdg. +3 dgt.				
Measurement rar	ge 0.5Hz or more ([] is displayed when frequency is less than 0.5Hz)				
Pulse width	1µs or more (DUTY ratio is 50%)				
With the filter ON					

With the filter ON, accuracy is defined only for frequencies 100Hz or less. (For ACV, DC+ACV)

General Specifications

Safety				
Maximum rated voltage between input terminals and ground		CAT III 1000V/ CAT IV 600V		
Maximum rated voltage between terminals		Between the V and COM terminals : 1000 V DC/AC		
Maximum fated current		een the mA and COM terminals : 600mA DC/600mA AC Between the A and COM terminals : 10A DC/10A AC		
Durability				
Drop proof		YES		
Operating temperature and humidi	ty*1	-15°C to 55°C		
Storage temperature and humidit	ty*2	-30°C to 60°C		
Dielectric strength		AC8.54kV (Between all input terminals and case)		
Applicable standards		Safety : EN61010, EMC: EN61326, Waterproof and dustproof: IP40		
*1 : -15°C to 55°C (5°F to 131°F), Up to 40°C (104°F): at 80%RH or less (non-condensating), 40°C to 45°C (104°F to 113°F): at 60%RH or less (non-condensating), 45°C to 55°C (113°F to 131°F): at 50%RH or less (non-condensating) *2 : 80%RH or less (non-condensating)				

Dimensions/Mass

93mm(W)×197mm(H)×53mm(D)(3.66"W 7.76"H 2.09"D Inch) / 650g (including batteries) (23 oz.)

Accessories _

TEST LEAD L9207-10 , Instruction Manual, LR6 alkaline battery×4

DT4281 only

DT4251/DT4252/DT4253



Accuracy Guaranteed for 1 Year @ $23 \pm 5^{\circ}C$ (73°F±41°F), 80% RH or less (no condensation)

DC Voltage	High precision 600mV range : DT4252 only			
Range	Accuracy	Input Impedance		
High precision 600mV range	±0.2 %rdg. ±5 dgt.	$10.2 M\Omega \pm 1.5 \%$		
600.0 mV	±0.5 %rdg. ±5 dgt.	$11.2M\Omega \pm 2.0\%$		
6.000 V		$11.2002 \pm 2.0.76$		
60.00 V	±0.3 %rdg, ±5 dgt.	$10.3M\Omega \pm 2.0\%$		
600.0 V	± 0.3 % rug. ± 3 ugi.	10 20 (0) + 1 5 9/		
1000 V		$10.2M\Omega \pm 1.5$ %		

AC voltage				
Panga	Accu	iracy	Innut Innu dan as	
Range 40 to 500Hz		500 or more to 1kHz	Input Impedance	
6.000V		±1.8 %rdg. ±3 dgt.	$11.2M\Omega \pm 2.0\% //100 pF$ or less	
60.00V	10.00% ada 12 dat		$10.3M\Omega \pm 2.0\% //100 pF$ or less	
600.0V	±0.9 %rdg. ±3 dgt.		10 2MO + 1 59/ //100 -E an land	
1000V			$10.2M\Omega \pm 1.5\% //100 pF$ or less	

AUTO V (Identification) DT4251,DT4253			4251,DT4253 only	
Range		Accuracy		Input Impedance
Kange	DC.	,40 to 500Hz	500 or more to 1kHz	input impedance
600.0 V	±2.0 %rdg. ±3 dgt.		±4.0 %rdg. ±3 dgt.	$900 k\Omega \pm 20\%$
Crest factor	3 up to 4000 counts and reduces linearly to 2 at 6000 counts.			at 6000 counts.
Accuracy specification range		For ACV, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range		
		With the filter ON the accuracy is not specified in 100Hz/500Hz or more		

DCA Measurement	60uA 60mA range: DT4253	only / 6A, 10A range : DT4252 only	
Range	Accuracy	Input Impedance	
60.00 µA	recuracy	mput impedance	
600.0 μA		1 kΩ±5 %	
6.000 mA	±0.8 %rdg. ±5 dgt.		
60.00 mA		15 Ω±40 %	
6.000 A			
10.00 A	±0.9 %rdg. ±5 dgt.	35 mΩ±30 %	

ACA Measu	rement		DT4252 only
Range	Accuracy		Input Impedance
Kange	40 to 500Hz	500 or more to 1kHz	input inipedance
6.000 A	±1.4 %rdg. ±3 dgt.	±1.8 %rdg. ±3 dgt.	35 mΩ±30 %
10.00 A	±1.4 %iug. ±5 ugi.	±1.8 %iug. ±5 ugi.	55 III22±50 %

 Crest factor
 3 up to 4000 counts and reduces linearly to 2 at 6000 counts.

 Accuracy specification range
 Minimum 1% of range; add ±5 dgt. when measuring 300 counts or less

Electric Charge	DT4251 only
Detection voltage range	Detection Target Frequency
80 VAC to 600 VAC	50Hz / 60Hz

During voltage detection, a continuous buzzer sounds and the red LED lights up.

Continuity Chec	k			
Range	А	ccuracy	Measurement Current	Open-terminal Voltage
600.0 Ω	±0.7 %rdg. ±5 dgt.		Approx. 200 µA	DC1.8 V or less
Continuity ON threshold Approx. 2		Approx. 25Ω or	less (continuous buzzer	sound, red LED lights)
Continuity OFF threshold		Approx.245Ω or	more	

Diode Check				
Range		Accuracy	Measurement Current	Open-terminal Voltage
1.500 V	±0.5 %rdg. ±5 dgt.		Approx. 0.5 mA	DC5.0 V or less
Forward threshold		Buzzer sounds intermittently at 0.15V to 1.5V, the red LED flashes		

DT4251,DT4253 only			
Accuracy			
40 to 1kHz			
±0.9 %rdg. ±3 dgt.			

Accuracy does not include the error of the clamp-on probe.
Crest factor
3 or less

Accuracy specification range Minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range

Range	Accuracy	Measurement Current	Open-terminal Voltage
600.0 Ω		Approx. 200 µA	
6.000 kΩ	1070/ada 15 dat	Approx. 100 µA	
60.00 kΩ	±0.7 %rdg. ±5 dgt.	Approx. 10 µA	1.8 V DC or less
600.0 kΩ		Approx. 1 µA	1.6 V DC 01 less
6.000 MΩ	±0.9 %rdg. ±5 dgt.	Approx. 100 nA	
60.00 MΩ	±1.5 %rdg. ±5 dgt.	Approx. 10 nA	
Accuracy guarantee condition After zero adjustment has been performed			

Capacitance Measurement					
Range		Accuracy	Measurer	nent Current	Open-circuit Voltage
1.000 µF			Approx. 1	0n/100n/1 μA	
10.00 µF		100/ada 15 dat	Approx. 1	00n/1μ/10 μA	
100.0 µF	3	=1.9 %rdg. ±5 dgt.	Approx. 1	µ/10µ/100 µA	1.8 V DC or less
1.000 mF			Approx. 10	μ/100μ/200 μΑ	
10.00 mF	±5.0 %rdg. ±20 dgt.		Approx.	100µ/200 µA	
Temperature					DT4253 only
Thermocouple Type Range			Ac	curacy	
K	K -40.0 to 400.0		°C	±0.5 %	ordg. ±2 °C

The optional K Thermocouple DT4910 is used. Accuracy does not include the error of the K thermocouple

Frequency	
Range	Accuracy
99.99 Hz	
999.9 Hz	1010/mlm 11.det
9.999 kHz	±0.1 %rdg. +1 dgt.
99.99 kHz (VAC Only)	

General Specifications.

Safety					
Maximum rated voltage between input terminals and ground	CAT III1000V/ CAT IV600V				
Maximum rated voltage between terminals	Between the V and COM terminals : 1000 V DC/AC				
Maximum rated current between terminals	Between the A and COM terminals : 10A DC/10A AC (DT4252 Only) Between the mA ,mAand COM terminals : 60mA DC (DT4253 Only)				
Durability					
Drop proof	YES				
Operating temperature and humidity	*1 -10°C to 50°C				

Operating temperature and humidity*1	-10°C to 50°C
Storage temperature and humidity*2	-30°C to 60°C
Dielectric strength	AC8.54kV (Between all input terminals and case)
Applicable standards	Safety : EN61010, EMC: EN61326, Waterproof and dustproof: IP42

*1: -10°C to 50°C(14°F to 122°F), Up to 40°C(104°F): at 80%RH or less(non-condensating), 40°C to 45°C (104°F to 113°F): at 60%RH or less(non-condensating), 45°C to 50°C (113°F to 122°F): at 50%RH or less (non-condensating)

*2:80%RH or less (non-condensating)

Dimensions/Mass

84mm(W)×174mm(H)×52mm(D)(3.31"W 6.85"H 2.05"D) 390g (including batteries and holster) (13.8 oz.)

Accessories .

TEST LEAD L9207-10 / Instruction Manual / LR03 Alkaline battery×4 Holster (attached to the instrument, with a test lead holder)

DT4221/DT4222


Display



while we wing angle display

Read measurements from any angle.

Hazard Prevention



White backlight ensures easy reading of measured values even in dark worksites.

conditions



Bar graph refreshes 40 times/second. Acts just like an analog meter to intuitively expose changes in the measured signal.

.... transformation deservices of

APS

CTER.

APS 💷

The screen flashes to indicate input overload and over-range



Designed for Effortless Handling

The A terminal is omitted to enhance safety

Omitting the unused current measurement terminal

helps to avoid operator faults such as short circuits,

breaker tripping and fires.



Small, light, and fits easily in a pocket.

RANGE · AUT

Over-range input indication


Test leads plug into the rear The display is not obscured by the leads when measuring.



Just wrap the leads and clip the probes at the back. Resume operation smoothly without tangled leads.



Operates on one battery Runs on one alkaline battery. Battery replacement is a snap.

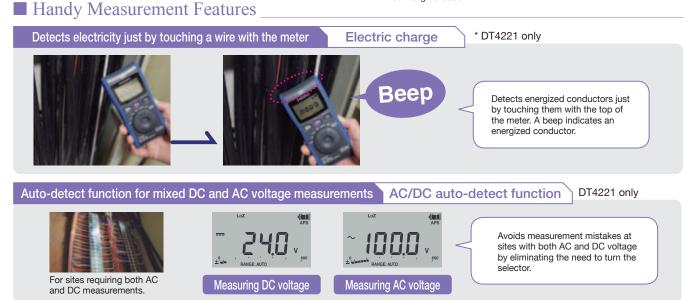

Accuracy Guaranteed for 1 Year @ $23 \pm 5^{\circ}C$ (73°F±41°F), 80% RH or less (no condensation)

DC Voltage			_	_				
Range		Accuracy				Input Impedance		
600.0 mV		±0.5 %rdg. ±5 dgt.			$11.2M\Omega \pm 2.0\%$			
6.000 V						$11.21 \text{VI} \text{L} 2 \pm 2.0 \%$		
60.00 V					$10.3M\Omega \pm 2.0\%$			
600.0 V						10.2	2M	$\Omega \pm 1.5$ %
AC Voltage								
D		Accuracy				Innut Innu dan sa		
Range	40 t	o 500Hz	500 or more to 1kHz Input Im			t Impedance		
6.000V			±2.5	%rdg. ±3 dgt. 11.2MΩ		Ω±	± 2.0%//100pF or less	
60.00V	±1.0 %	±1.0 %rdg. ±3 dgt.		.0 %rdg. ±3 dgt.		$10.3M\Omega \pm 2.0$ %//100pF or less		
600.0V			12.0	/orug. ±5	ugi.	$10.2M\Omega \pm 1.5$ %//100pF or less		
Crest factor	3 up to	3 up to 4000 counts and reduces linearly to 2 at 6000 counts.				000 counts.		
				of range;	add ⊧	5 dgt. w	hei	n measuring at
Accuracy specification range		w 5% of ran	~					
-F8-	With th	e filter ON,th	ne accu	racy is no	t spec	ified in 10)0F	Iz/500Hz or more
AUTO V (Identii	ication)							DT4221 only
		Accuracy						
Range	DC	DC,40 to 500Hz 500 or			more	more to 1kHz Input Impedance		
600.0 V	±2.0	±2.0 %rdg. ±3 dgt.			0 %rdg. ±3 dgt.			$900k\Omega \pm 20$ %
Crest factor	3 up to	3 up to 4000 counts and reduces linearly			ly to 2 at	60	000 counts.	
Accuracy	1% , minimum 1% of range; add ± 5 dgt. when measuring at or 5% of range							
specification range		With the filter ON, the accuracy is not specified in 100Hz/500Hz or more						
					p			
Electric Charge								DT4221 only
Detectio	n Voltage l	Range		Detection Target Frequency				
80 V A	C to 600 V	' AC		50Hz / 60Hz				
During voltage detection	n, a continuc	ous buzzer sou	nds.					
Continuity Check	(
Range		Accuracy		Meas	Measurement Current			Open-terminal Voltage
600.0 Ω	±1	±1.0 %rdg. ±5 dgt.		Ap	prox.	200 µA		DC1.8 V or less
Continuity ON the	nreshold	Approx. 2	5Ω or	less (cont	inuou	s buzzer s	sou	nd)
Continuity OFF t		Approx.24						· · · · · · · · · · · · · · · · · · ·
								574000
Diode Check			-			a		DT4222 only
Range		Accuracy				Current	(Open-terminal Voltage
1.500 V	±0.9 %rdg. ±5 dgt.			Appro	ox. 0.	5 mA		DC2.5 V or less

Diode Check			DT4222 only		
Range	Accuracy	Measurement Current	Open-terminal Voltage		
1.500 V	±0.9 %rdg. ±5 dg	t. Approx. 0.5 mA	DC2.5 V or less		
Forward threshold	Buzzer sounds in	Buzzer sounds intermittently at 0.15V to 1.5V			

Resistance Measurement DT4222 only							
Range		1	Accuracy		Measurement Current	Open-terminal Voltage	
600.0 Ω					Approx. 200 µA	-	
6.000 kΩ					Approx. 100 µA		
60.00 kΩ		±0.9 %rdg. ±5		gt.	Approx. 10 µA	1.8 V DC or less	
600.0 kΩ					Approx. 1 µA	1.8 V DC or less	
6.000 MΩ					Approx. 100 nA		
60.00 MΩ		±1.5 %rdg. ±5 dgt.		Approx. 10 nA]		
Accuracy guarantee condition After zero adjustment has been performed				ed			
Capacitance Measurement DT4222 onl					DT4222 only		
Range		Accuracy		Me	easurement Current	Open-terminal Voltage	
1.000 µF				Appro	ox. 10n/100n/1 μA		
10.00 µF		100/ada	15 3-4	Appro	ox. 100n/1μ/10 μA		
100.0 μF				Appro	ox. 1μ/10μ/100 μA	1.8 V DC or less	
1.000 mF				Approx	к. 10µ/100µ/200 µА		
10.00 mF	-	±5.0 %rdg. =	±20 dgt.	. Approx. 100μ/200 μA			
Frequency							
Range				A	Accuracy		
99.99 Hz							
		±0.1 %rdg. +2 dgt.					

General Specifications

9.999 kHz

Salety				
Maximum rated voltage between input terminals and ground	CAT III 600V/ CAT IV300V			
Maximum rated voltage between terminals	Between the V and COM terminals : 600 V DC/AC			
Durability				
Drop proof	YES			
Operating temperature and humidity*1	-10°C to 50°C			
Storage temperature and humidity*2	-30°C to 60°C			
Dielectric strength	AC7.06kV (Between all input terminals and case)			
Applicable standards	Safety : EN61010, EMC: EN61326, Waterproof and dustproof: IP42			
*1 -10°C to 50°C(14°F to 122°F) Up to 40°C(104°F); at 80%RH or less(non-condensating)				

*1: -10°C to 50°C (114°F to 122°F), Up to 40°C (104°F): at 80% RH or less 40°C to 45°C (104°F to 113°F): at 60% RH or less (non-condensating), 45°C to 50°C (113°F to 122°F): at 50% RH or less (non-condensating) *2: 80% RH or less (non-condensating)

Dimensions/Mass 72mm(W)×149mm(H)×38mm(D) (2.83"W 5.87"H 1.50"D) 190g (including batteries and holster) (6.7 oz.)

Accessories

TEST LEAD DT4911 / Instruction Manual / LR03 Alkaline battery×1 Holster (attached to the instrument, with a test lead holder.)


Measurement categories (Overvoltage categories)

To ensure safe operation of measurement products, IEC 61010 establishes safety standards for various electrical environments, categorized as CAT II to CAT IV, and called measurement categories. These are defined as follows.

CAT II : Primary electrical circuits in equipment connected to an AC electrical outlet by a power cord (portable tools, household appliances, etc.) CAT III : Primary electrical circuits of heavy equipment (fixed installations) connected directly to the distribution panel, and feeders from the distribution

panel to outlets.

CAT IV : The circuit from the service drop to the service entrance, and to the power meter and primary overcurrent protection device (distribution panel).

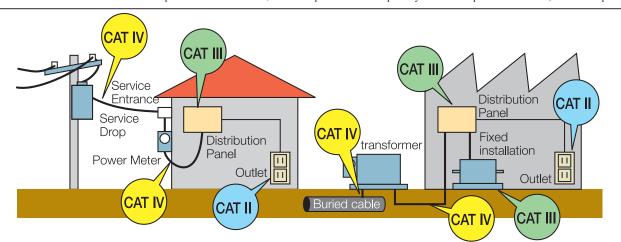

Higher-numbered categories correspond to electrical environments with greater momentary energy, so a measurement product designed for CAT III environments can endure greater momentary energy than one designed for $\mathbf{CAT}\ \mathrm{II}$.

